


FDC39 Dental Chair



FDC38H (高配型) DENTAL UNIT

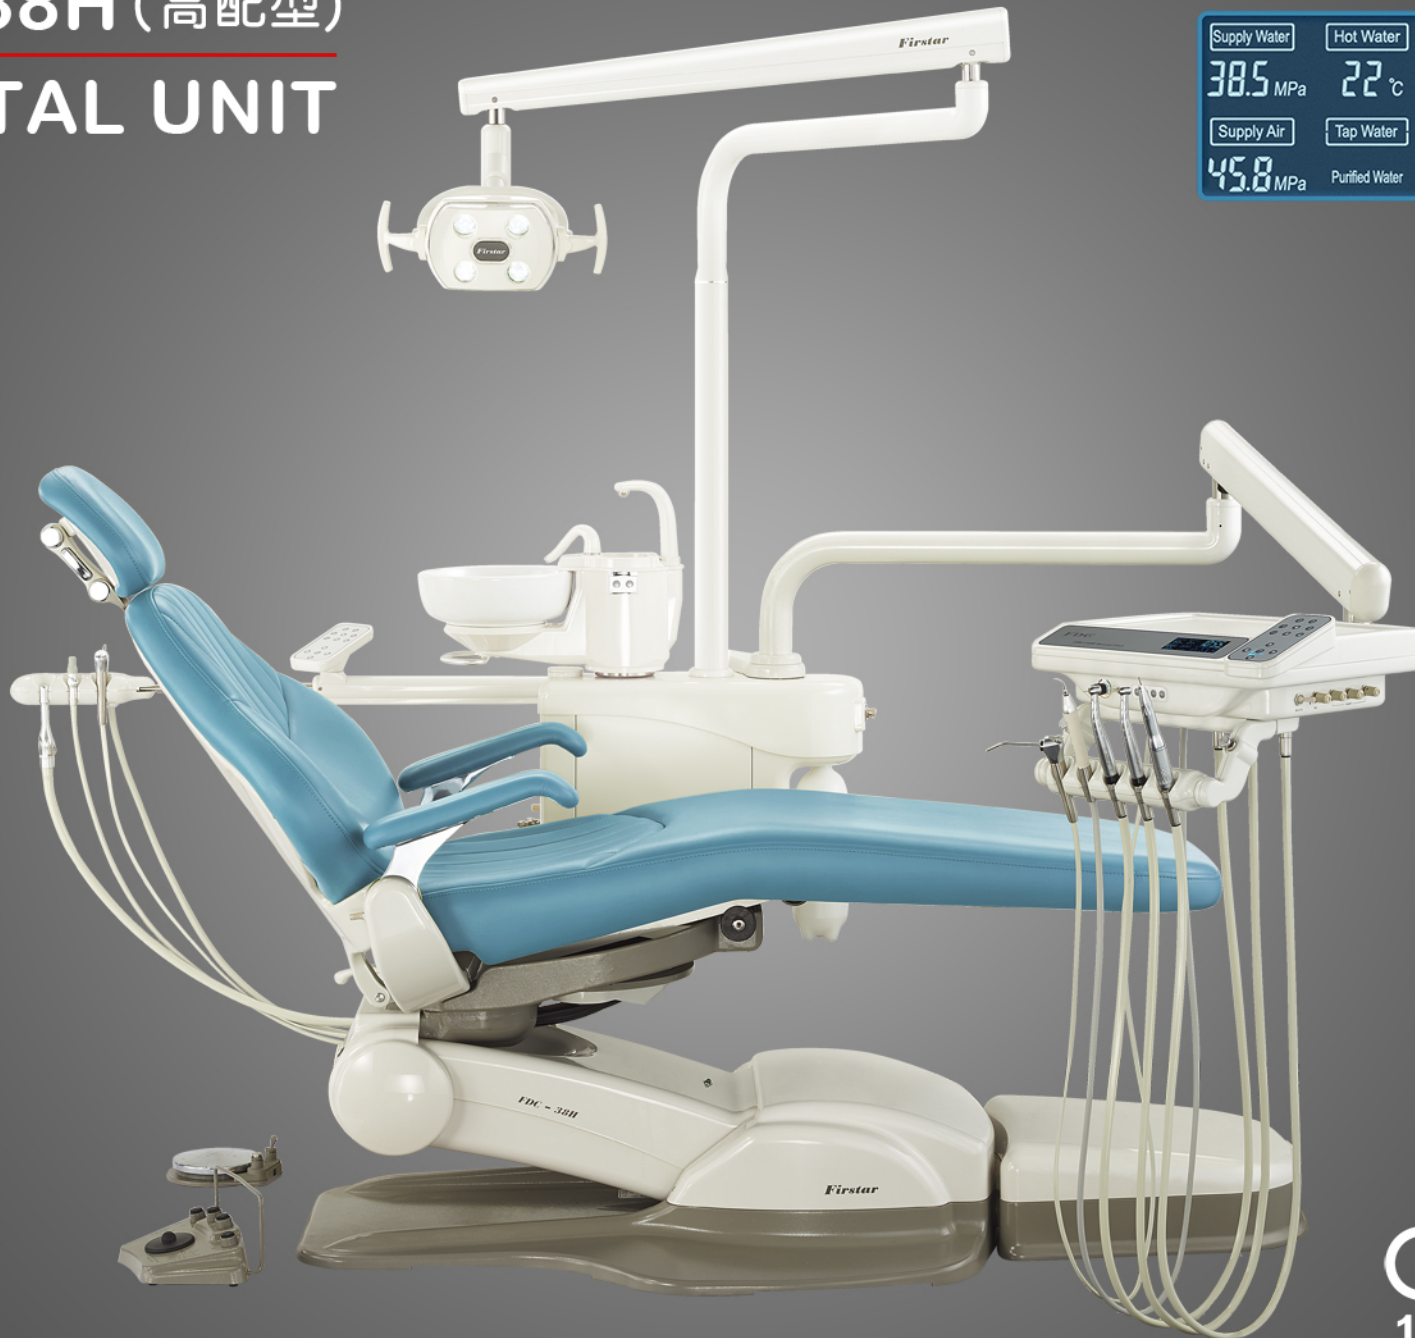

Supply Water	Hot Water	8:30	
38.5 MPa	22 °C	DAY	MONTH DATE TEMP
Supply Air	Tap Water	MON 1-3 24°C	
45.8 MPa	Purified Water		



FDC39H (高配型) DENTAL UNIT



Supply Water	Hot Water	8:30	
38.5 MPa	22 °C	DAY	MONTH DATE TEMP
Supply Air	Tap Water	MON 1-3 24°C	
45.8 MPa	Purified Water		



FDC50H

DENTAL UNIT



Supply Water	Hot Water	8:30		
38.5 MPa	22 °C	DAY	MONTH	DATE
Supply Air	Tap Water	TEMP		
45.8 MPa	Purified Water	MON	1-3	24°C



Doctor stool and Assistant stool



LED-1 Dental Light



LED-2 Dental Light



LED-3 Dental Light

